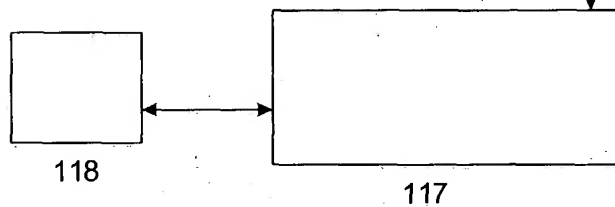


Fig. 1



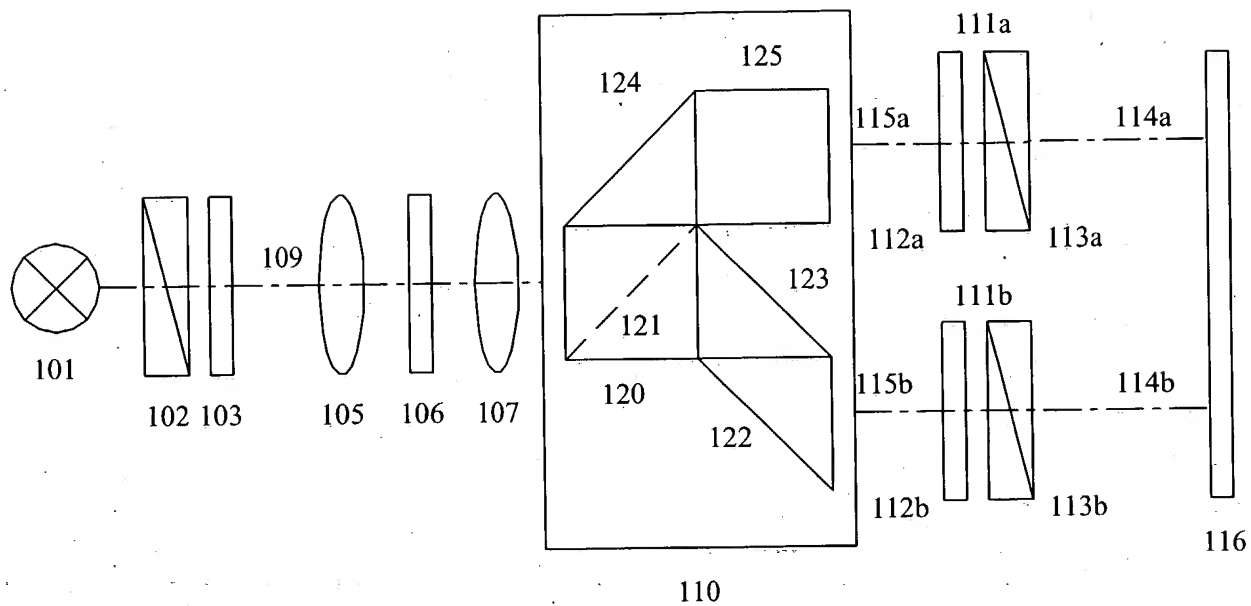


Fig. 2a

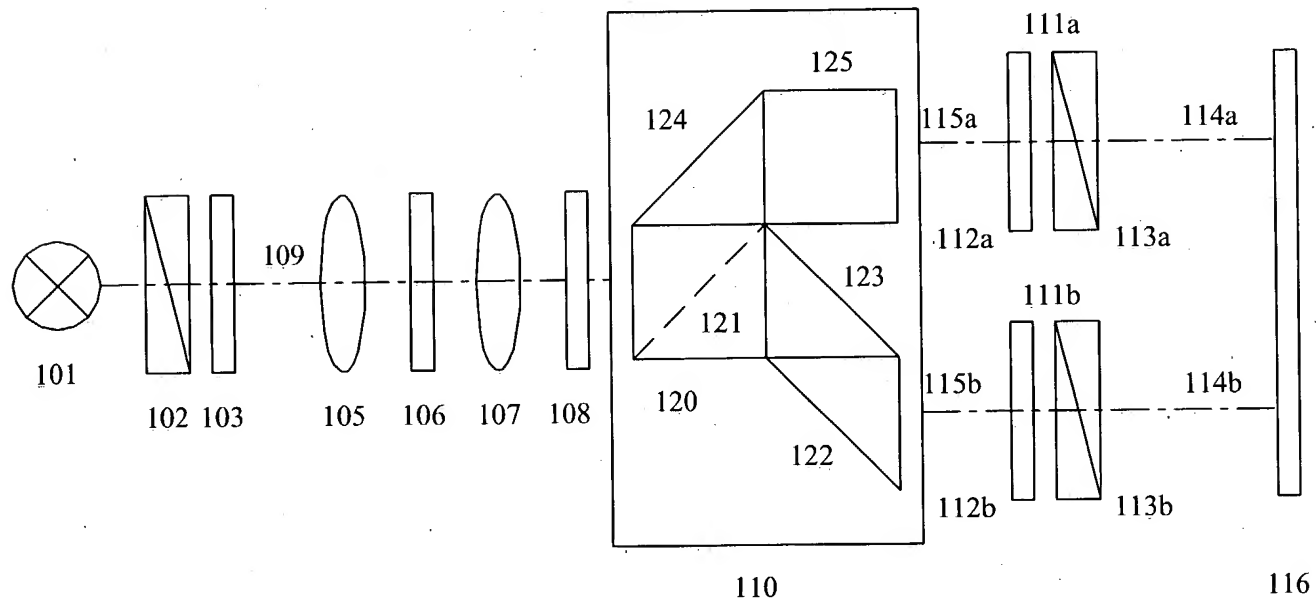


Fig. 2b

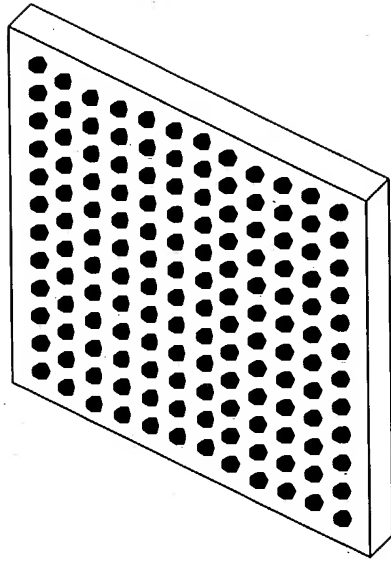


Fig. 3

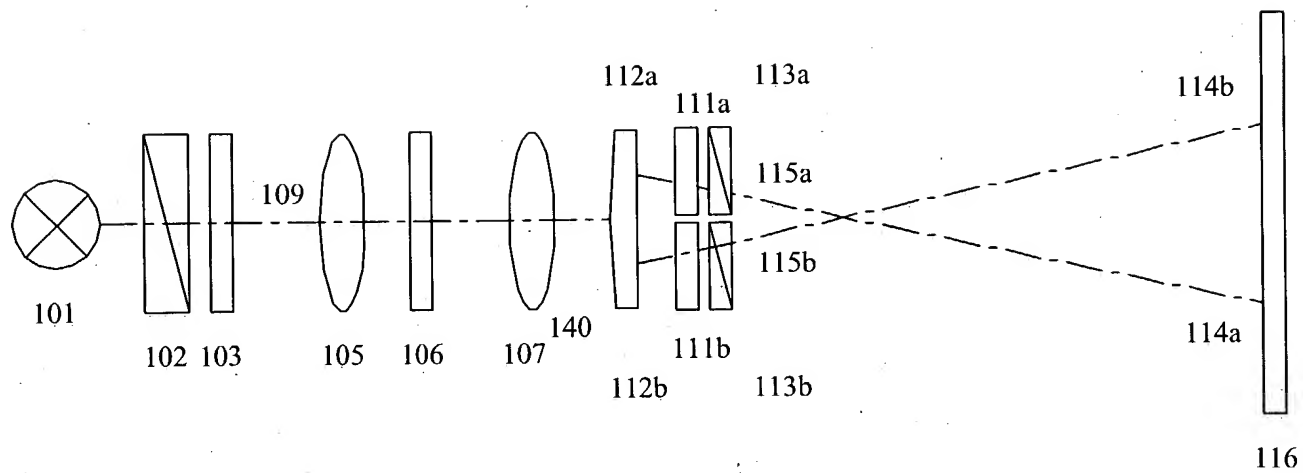


Fig. 4a

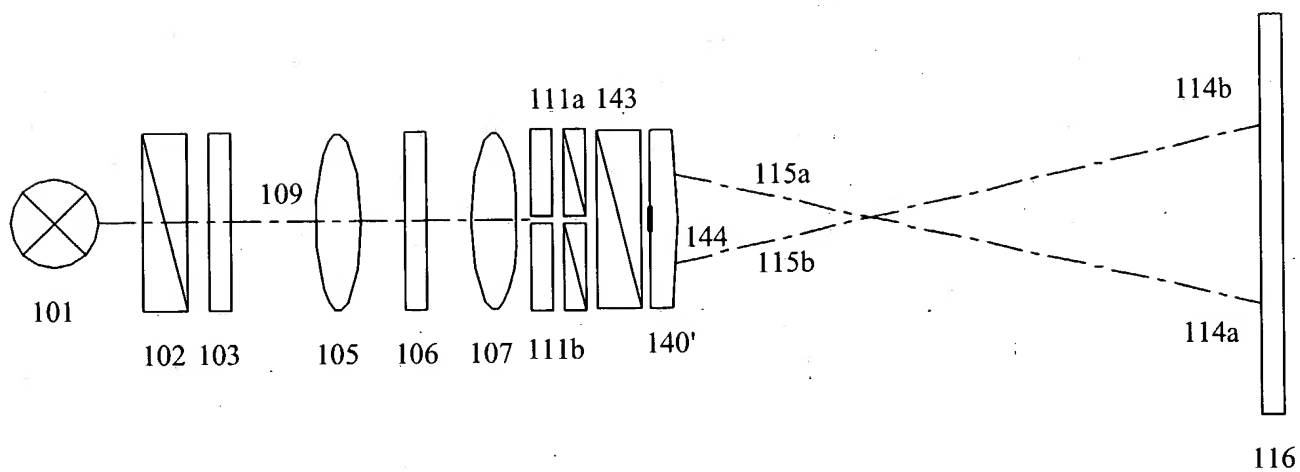


Fig. 4b

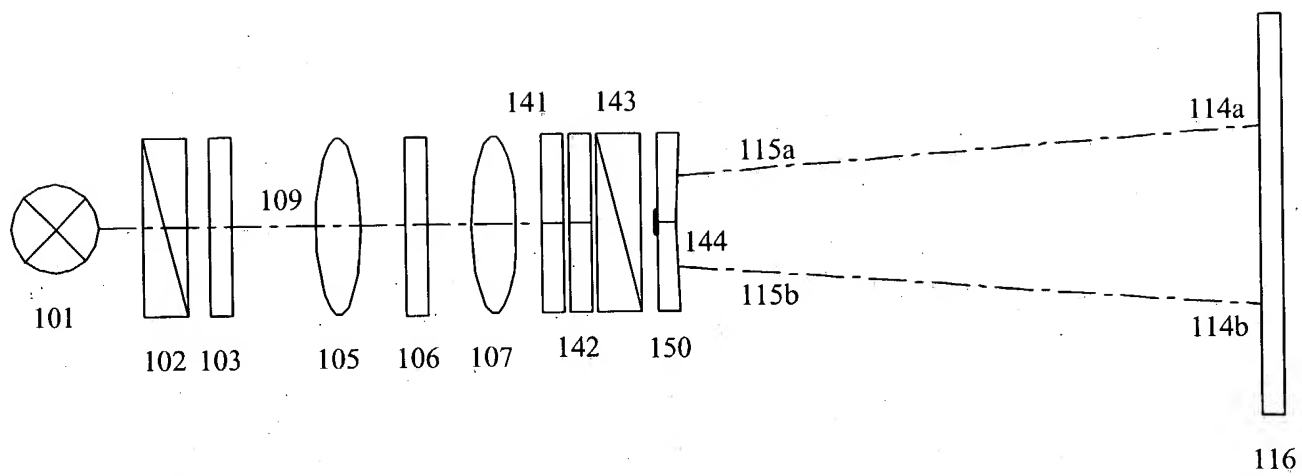


Fig. 5

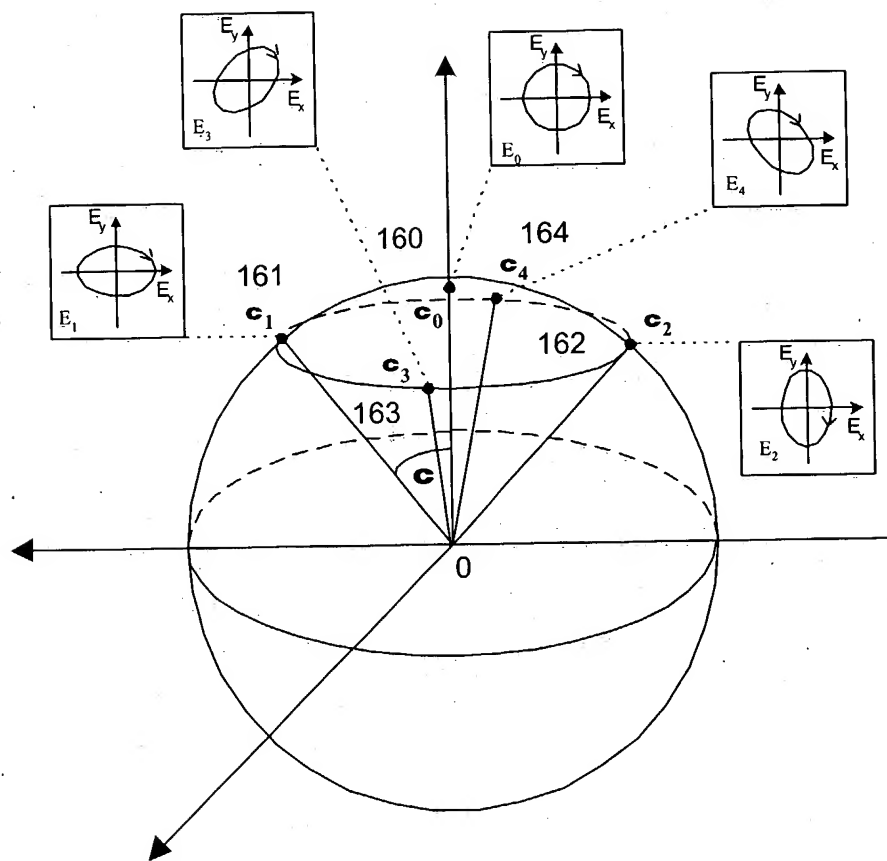


Fig. 6

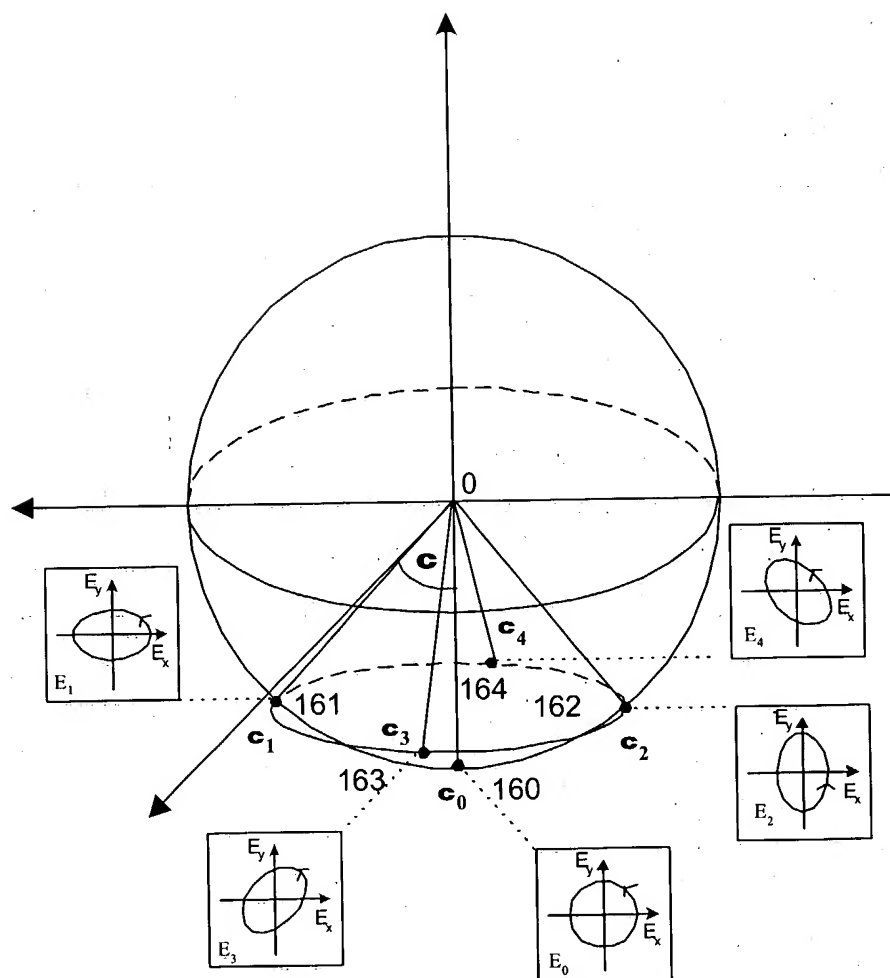


Fig. 7

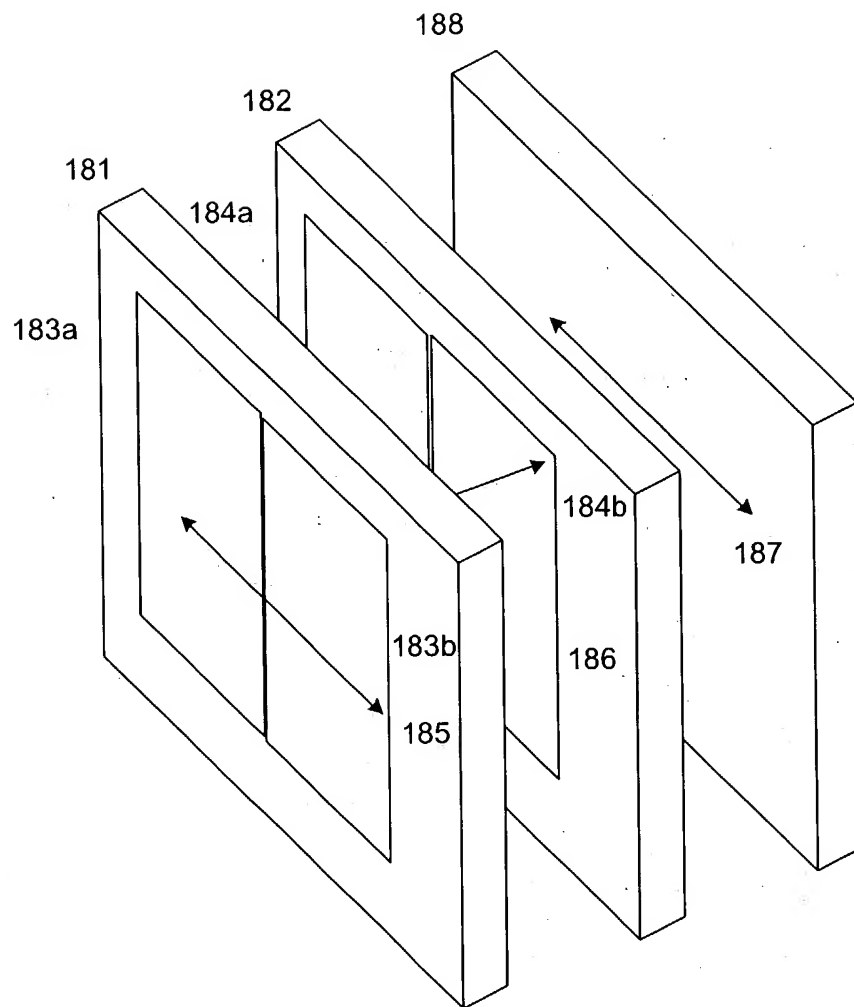


Fig. 8a

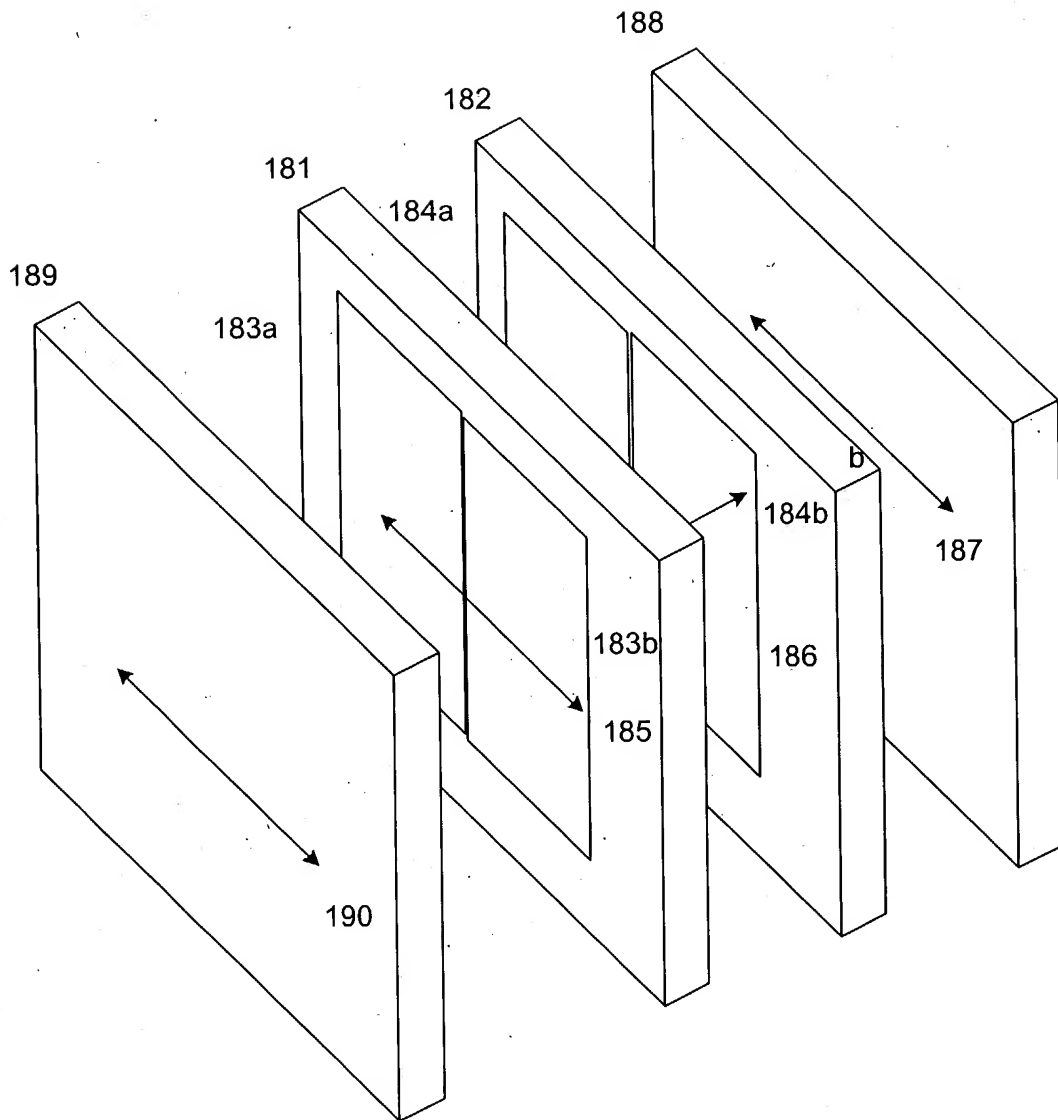


Fig. 8b

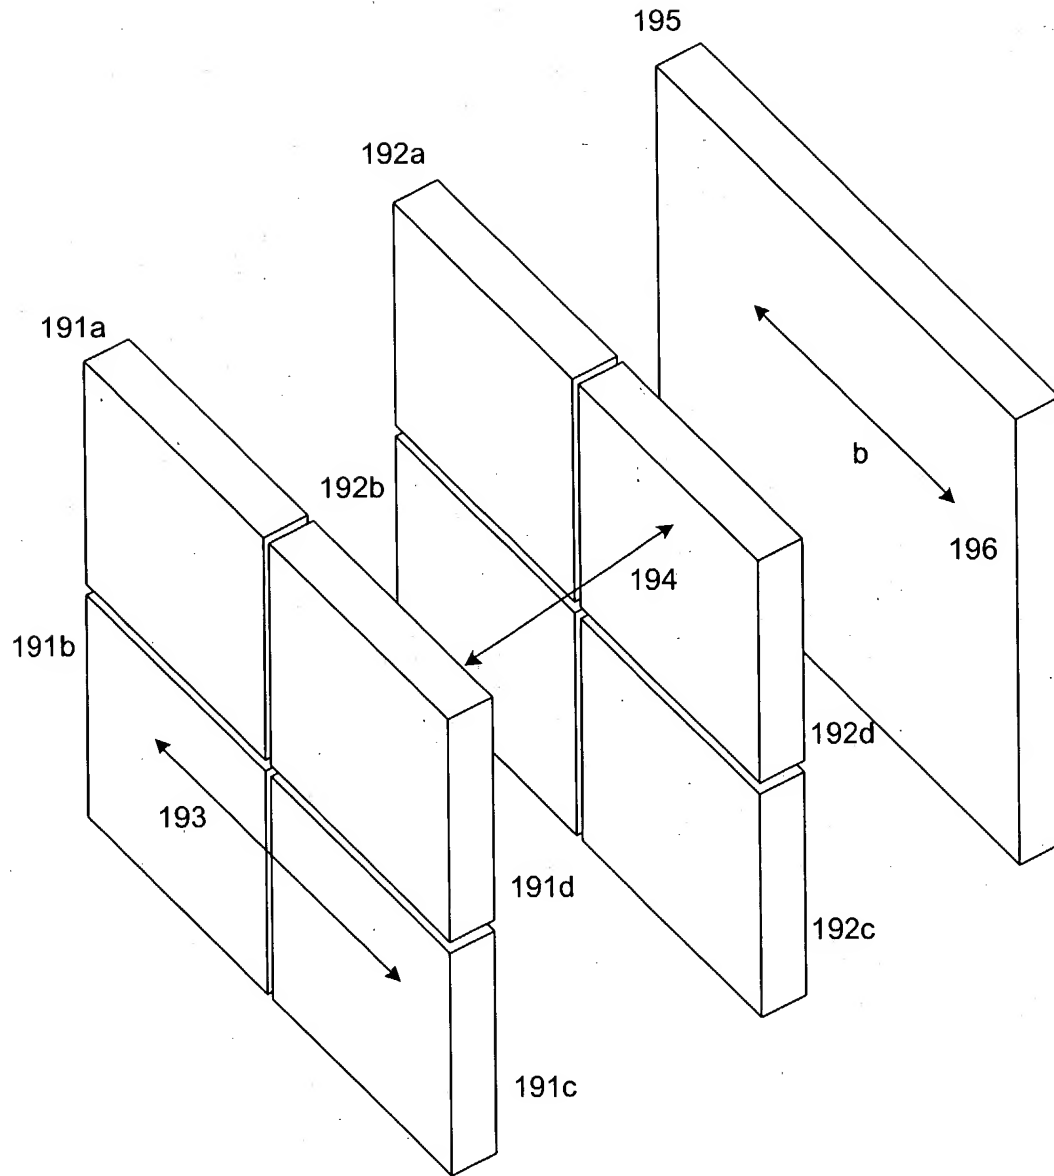


Fig. 9

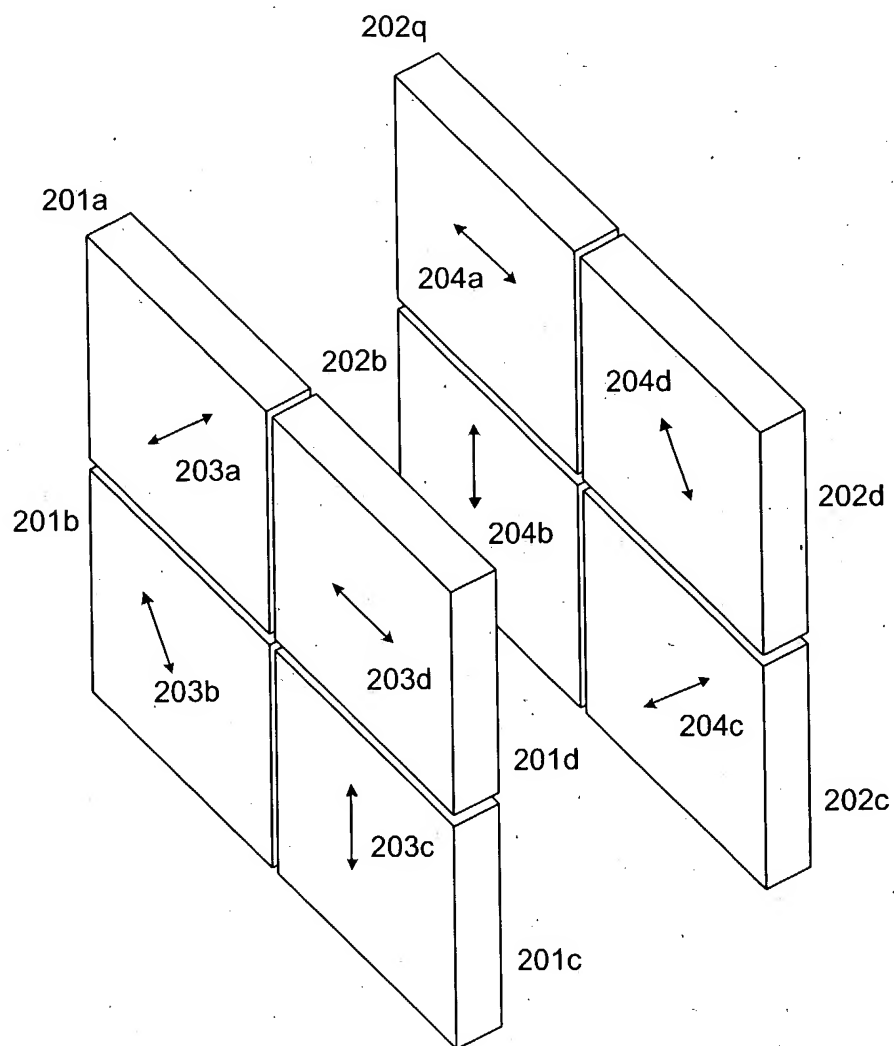


Fig. 10

Acquisition sequence

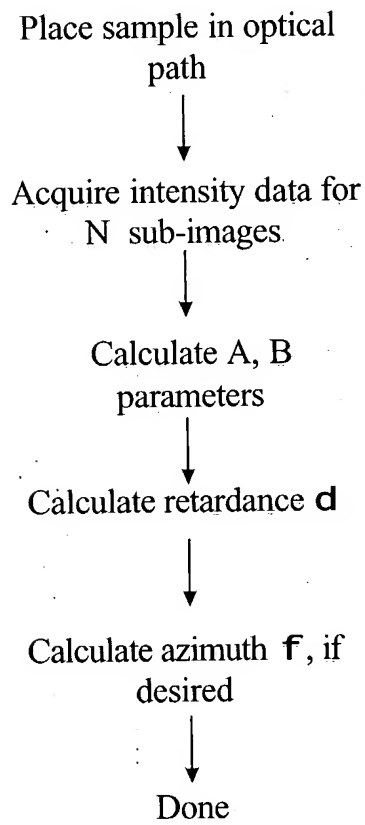


Fig. 11

Acquisition sequence with background measurement

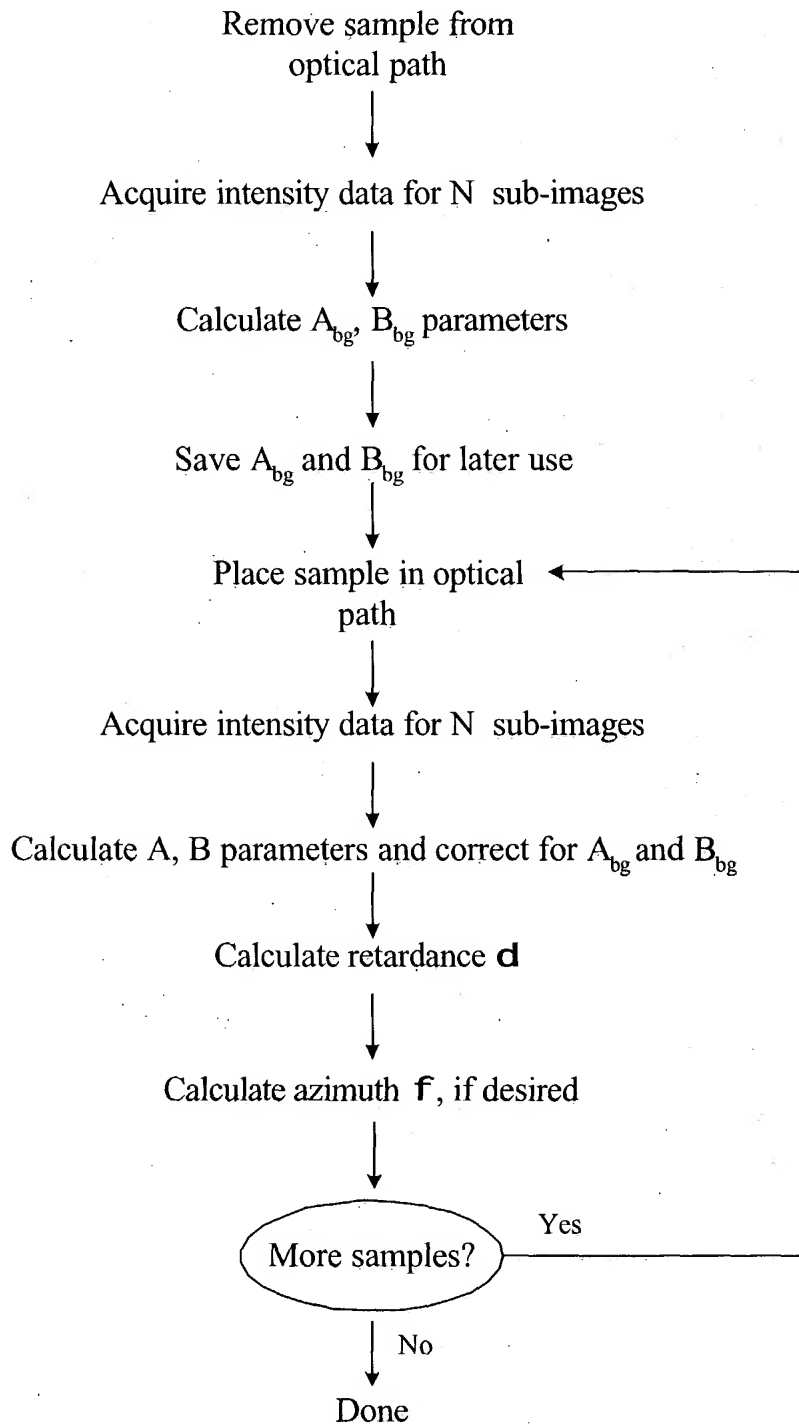


Fig. 12

Acquisition sequence with calibration measurement

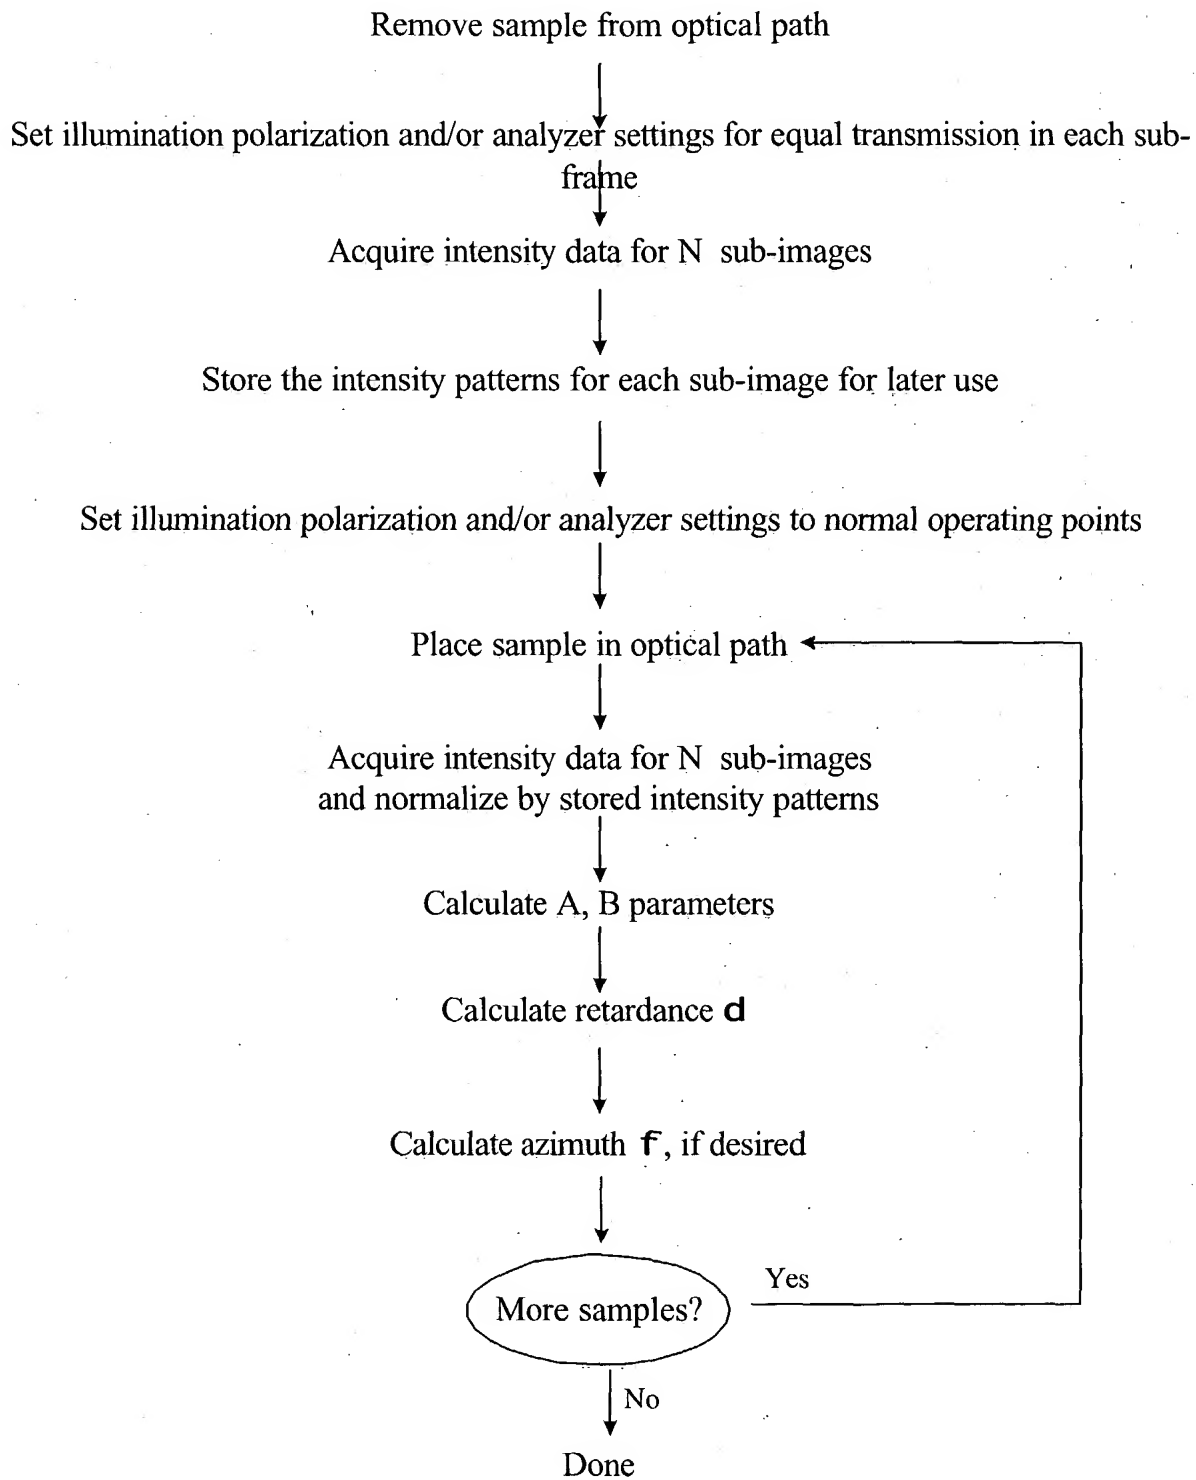


Fig. 13

Acquisition sequence with calibration measurement and background correction

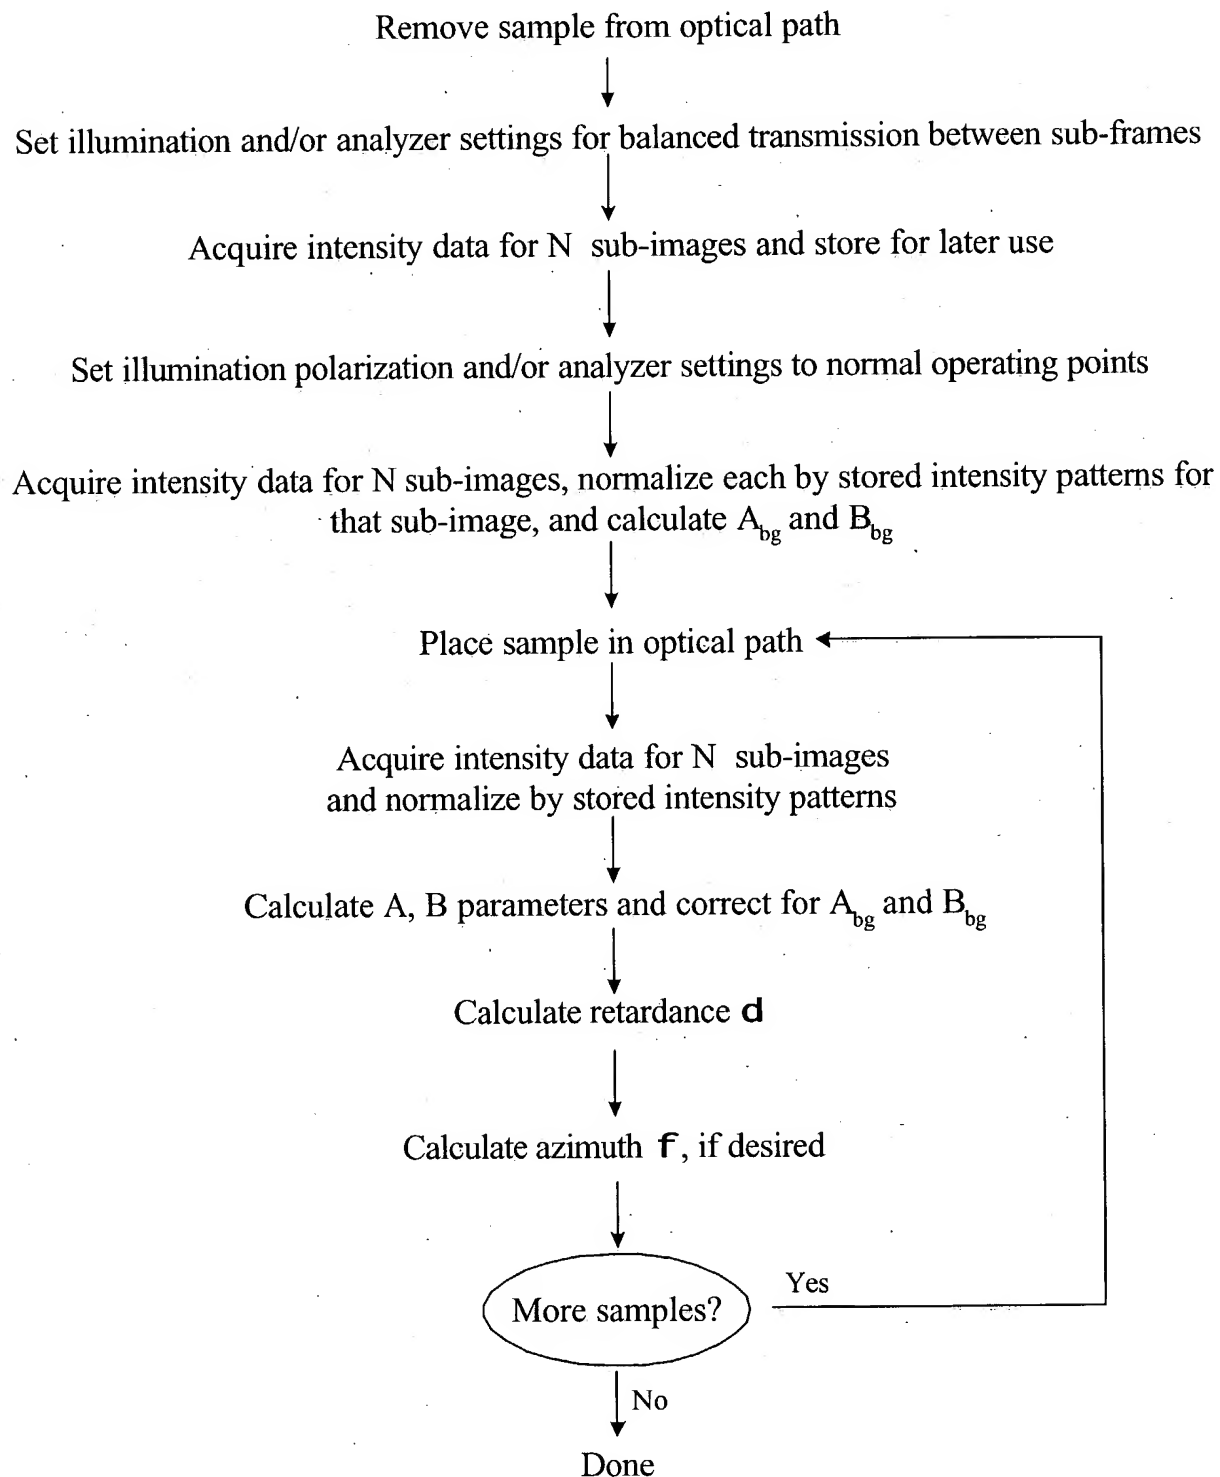


Fig. 14